



Ultrasensitive determination of β -conglutin food allergen by means an aptamer assay based on inductively coupled plasma mass spectrometry detection

Daniel Torregrosa^a, Miriam Jauset-Rubio^b, Raquel Serrano^a, Marketa Svobodová^b, Guillermo Grindlay^{a,*}, Ciara K. O'Sullivan^{b,c}, Juan Mora^a

^a University of Alicante, Department of Analytical Chemistry, Nutrition and Food Sciences, PO Box 99, 03080, Alicante, Spain


^b INTERFIBIO Consolidated Research Group, Department of Chemical Engineering, Universitat Rovira i Virgili, 43007, Tarragona, Spain

^c Institució Catalana de Recerca i Estudis Avançats (ICREA), 08010, Barcelona, Spain

HIGHLIGHTS

- Different aptamer assays based on ICP-MS detection are evaluated for β -conglutin determination.
- Biotinylated aptamers with Streptavidin-AuNPs afford better results than AuNPs-thiolated ones.
- Conventional ICP-MS detection mode provides better LoDs than the single particle one.
- The use of ICP-MS results in a 10 to 100-fold LoD improvement with regard other detection approaches.

GRAPHICAL ABSTRACT

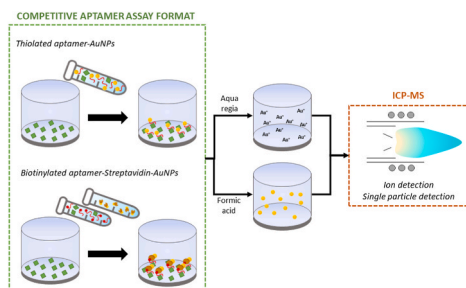

ARTICLE INFO

Handling Editor: Xiu-Ping Yan

Keywords:

β -conglutin
Aptamer assay
Nanoparticles
Single particle
Inductively coupled plasma mass spectrometry

ABSTRACT

The overall objective of this work is the evaluation of different competitive aptamer assays based on inductively coupled plasma mass spectrometry (ICP-MS) detection for the determination of β -conglutin (food protein allergen from lupin) in flour samples. To this end, two competitive aptamer assay schemes were developed using either thiolated aptamers chemisorbed onto gold nanoparticles (AuNPs) or biotinylated aptamers linked to streptavidin-AuNPs. The influence of ICP-MS detection mode (i.e., conventional vs single particle) on assay performance was explored. In the case of the thiolated aptamer, the limit of detection (LoD) obtained using the single particle mode was improved 2-fold as compared to the LoD provided by the conventional mode. With regards to the biotinylated aptamer, the use of the conventional mode provided a 5-fold improvement of LoD as compared to that obtained for the single particle one. Using the optimized conditions, the best LoD of 2 pM was obtained with the biotinylated aptamer operating with conventional ICP-MS detection. When compared to previous reports using the same aptamer in a competitive assay, the developed method significantly improved the LoD by at least an order of magnitude. Different flour samples containing lupin were successfully analyzed according to European Conformity guidelines for the analysis of food contaminants.

* Corresponding author.

E-mail address: guillermo.grindlay@ua.es (G. Grindlay).

<https://doi.org/10.1016/j.aca.2023.341042>

Received 24 November 2022; Received in revised form 1 March 2023; Accepted 2 March 2023

Available online 3 March 2023

0003-2670/© 2023 The Authors. Published by Elsevier B.V. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

1. Introduction

Lupin is a leguminous plant employed in the food industry as an alternative to gluten containing wheat (e.g., breads, cookies, pasta, etc.) [1,2], and there have been increasing reports of allergic reactions following ingestion of lupin [3,4]. Lupin-based allergenicity is related to the globulin protein fraction, particularly β -conglutin, and this protein has thus been designated as the Lup an 1 allergen by the International Union of Immunological Societies (IUIS) [5]. Additionally, lupin has been added to the list of substances requiring mandatory advisory labelling on foodstuffs sold in the European Union [6].

Several analytical methodologies have been developed for the determination of β -conglutin in food [4,7–9] including commercially available immunoassays. As an alternative to these techniques, aptamer assays based on different detection methods are attractive due to their simplicity, specificity, and potential high sample throughput [4,10–17]. An example of this was reported by Svobodová et al. [14] who proposed an ultrasensitive competitive aptamer assay for the determination of β -conglutin in lupin flour based on a combination of aptamer detection with the polymerase chain reaction (PCR), achieving a LoD as low as 85 pM.

Inductively coupled plasma mass spectrometry (ICP-MS) is a well-established technique for elemental analysis at ultratrace levels in many different fields due to its outstanding analytical capabilities (i.e., limits of detection in the ng-pg L⁻¹ level, large dynamic range, multi-elemental and multi-isotopic capabilities and high robustness, among others). Furthermore, this technique also allows the analysis of organic molecules provided that an element detectable by means of ICP-MS is naturally present or is intentionally attached to analyte structure through the formation of chemical bond or non-covalent interactions [18]. Thus, ICP-MS has been extensively used as a highly sensitive detector for immunoassays using element-tagged antibodies [19]. Basically, after the immunoassay is completed, the immunocomplex is decomposed with acids and, then, the resulting mixture is directly introduced into the plasma where the element tag is ionized providing a signal that is proportional to analyte levels. Over the years, different element tags have been proposed but metallic nanoparticles (NPs) are usually preferred since they show a great potential for improving sensitivity and limits of detection (LoD) due to the significant number of atoms present in each NP [18,19]. Moreover, this type of tags allows the use of single particle mode for analyte detection (spICP-MS) [20]. In this case, a diluted organic/acid solution is employed to elute NPs without damage and the suspension is introduced into the plasma. By operating microsecond dwell times, each NP atomized and ionized within the plasma generates a single pulse of intensity. The number of pulses can be correlated to the concentration of the NPs in suspension and, hence, analyte levels. Several reports have highlighted that, for non-competitive bioassays, this mode can improve the LoD, and sample throughput as compared to conventional ICP-MS detection [21–23]. So far, immunoassays based on ICP-MS detection have extensively been employed in clinical analysis for ultrasensitive determination of proteins, hormones, enzymes and even cells [18,19,24], and have also been successfully employed in food security applications for monitoring food allergens [25], antibiotics [26] and toxins [27,28].

Despite methodological similarities with immunoassays, there has been much fewer reports detailing the use of aptamer assays based on ICP-MS detection [29–32], particularly for food security applications. The goal of this work is to develop a new procedure for ultrasensitive β -conglutin determination in foods by the combined use of an aptamer-based assay and ICP-MS detection. To this end, two competitive aptamer assay schemes have been developed using either thiolated aptamers chemisorbed onto gold nanoparticles (AuNPs) or biotinylated aptamers linked with streptavidin-AuNPs (SA-AuNPs). For both approaches, the influence of ICP-MS detection mode (i.e., conventional vs single particle) on assay performance was evaluated. Finally, the analytical methodologies developed have been applied to the

determination of β -conglutin in chickpea and soy flour samples spiked with lupin.

2. Materials and methods

2.1. Reagents and materials

All solutions were prepared using ultrapure water (Milli-Q water purification system, Millipore Inc., Paris, France).

Polyethylene glycol sorbitan monolaurate (Tween 20), chloroauric acid, trisodium citrate and streptavidin from *Streptomyces avidinii* were purchased from Sigma-Aldrich (Steinheim, Germany). Bovine serum albumin (BSA) was obtained from Biowest (Nuaillé, France) whereas phosphate buffer saline (PBS) tablets and F16 maxisorp polystyrene microtiter plates were obtained from Thermo Fisher Scientific (Roskilde, Denmark). Iridium 1000 mg L⁻¹ and Au 1000 mg L⁻¹ stock solutions were provided by Merck (Darmstadt, Germany). Thiourea, 69% w w⁻¹ nitric acid, 35% w w⁻¹ hydrochloric acid and 85% w w⁻¹ formic acid were purchased from Panreac (Barcelona, Spain). Gold nanoparticles (nominal diameter 40 nm) were obtained from BBI solutions (Cardiff, United Kingdom).

2.2. Oligonucleotides

A β -conglutin aptamer (5'-agc tcc aga aga taa att aca ggg gcc ggg gtc gct cag gca agg ggt tga cct gtc gta ggg att gtt tta aca act agg ata cta tga ccc c-3') previously selected by Jauset-Rubio et al. [15,16,33] and employed in diverse assay formats [34], was used in this work. This aptamer is highly specific against β -conglutin and it shows a limited affinity against other β -conglutin fractions (i.e., α - and γ -) and proteins present in flour samples [33]. Two different versions of this aptamer containing either a thiol or a biotin at 5' were supplied by Biomers (Ulm, Germany).

2.3. β -conglutin standards preparation

Globulin proteins from *Lupinus albus* seeds were extracted with dilute salt solutions, followed by isolation of different globulin fractions by anion-exchange chromatography and size exclusion chromatography by Sephacryl-200 HR linked to a peristaltic pump [8], as previously reported but with some minor modifications. During the globulin proteins extraction, the pellet was left to air dry overnight instead of 72 h and the dialysis step was replaced by the use of a Microcon centrifugal filter to change the buffer and concentrate the obtained extract. Diethylaminoethanol fast flow sepharose resin was used for the anion-exchange chromatography following the program detailed in Table S1. Each fraction was collected after 4 min.

2.4. Solutions and buffers

β -conglutin detection by means of ICP-MS was carried out using two different element tagging schemes based on the use of 40 nm AuNPs. The first one was based on the direct chemisorption of a thiolated aptamer onto AuNPs, carried out following the method described by Jauset-Rubio et al. [15] The second approach was based on linking a biotinylated aptamer with SA-AuNPs. This latter compound was prepared combining citrate-stabilized AuNPs (optical density (OD) of 1) with 12.5 μ g mL⁻¹ streptavidin followed by a blocking step with BSA 1% w V⁻¹. The suspension was then centrifuged at 15000 rpm (Eppendorf Centrifuge 5417R, Spain) for 30 min, washed three times with 10% w w⁻¹ sucrose, 5 mM borate buffer pH 8.8 and 1% w V⁻¹ BSA, and resuspended with the same mixture (final OD 10).

The following media were employed for the incubation steps: (i) phosphate-buffered saline (PBS; 10 mM phosphate, 137 mM NaCl, 2.7 mM KCl, pH 7.4); (ii) carbonate buffer solution (15 mM Na₂CO₃ and 35 mM NaHCO₃, pH 9.6); (iii) washing medium (PBS-Tween; PBS + 0.05% V V⁻¹ Tween 20); (iv) binding buffer (PBS + 1.5 mM MgCl₂) – this is the

buffer that was used in the selection of the aptamer; and (v) blocking medium (2% w V⁻¹ BSA in PBS-Tween).

Finally, two different elution media were employed according to the ICP-MS detection mode. A diluted aqua regia (4% V V⁻¹ nitric acid and 12% V V⁻¹ hydrochloric acid) solution was employed to digest AuNPs for conventional ICP-MS measurements. For spICP-MS, NPs were released from the microtiter plate using a 1 M formic acid solution.

2.5. Aptamer assay procedures

The determination of β -conglutin by ICP-MS is based on the competitive aptamer assay described by Jauset-Rubio et al. [16] in which varying amounts of free β -conglutin inhibit the binding of specific modified aptamers to the solid phase coated with β -conglutin. Different aptamer assay procedures (i.e., thiolated vs biotinylated aptamers) and ICP-MS detection modes were tested using AuNPs as element tags (see Fig. 1).

2.5.1. Thiolated aptamer assay

For this assay (Fig. 1A), samples or β -conglutin standards were mixed with the thiolated aptamer-AuNPs suspension and incubated in binding buffer for 15 min at room temperature (step 1a). In parallel, the polystyrene microtiter plate wells were coated with 50 μ L of the appropriate β -conglutin concentration in 50 mM carbonate buffer. After a 30 min incubation at room temperature, wells were washed three times with PBS-Tween and blocked with blocking medium for 30 min at room

temperature. Subsequently, 50 μ L of the β -conglutin/thiolated aptamer-AuNPs mixture were transferred to the plate wells for another incubation step of 15 min at room temperature (step 2a). Finally, the plate was washed five times with PBS-Tween in order to eliminate β -conglutin-thiolated aptamer-AuNPs complexes present in the solution as well as the excess of the thiolated aptamer-AuNPs.

2.5.2. Streptavidin-AuNPs/biotinylated aptamer assay

In this approach (Fig. 1B), samples or β -conglutin standards were mixed with the biotinylated-aptamer solution and incubated in binding buffer for 15 min at room temperature (step 1b). In parallel, the polystyrene microtiter plate wells were coated, washed, and blocked as described in Section 2.5.1. In the following step, 50 μ L of the β -conglutin/biotinylated aptamer mixture was added to the coated wells and incubated for 15 min at room temperature (step 2b). After washing three times with PBS-Tween, the microtiter plates were sequentially incubated with 50 μ L of a 5 μ g mL⁻¹ SA-AuNPs suspension (OD 0.1) prepared in PBS-Tween for 15 min at room temperature (step 3b).

Irrespective of the aptamer assay, two different ICP-MS detection strategies were evaluated for the determination of β -conglutin: (i) conventional ICP-MS mode (Au⁺ signal detection). For this approach, AuNPs were digested for 3h with 150 μ L of the acidic digestion mixture and spiked with 50 μ L of a 1.0% w V⁻¹ thiourea solution containing 10 μ g L⁻¹ Ir as internal standard; and (ii) spICP-MS mode. In this case, AuNPs were released from the plate surface with 300 μ L of 1 M formic acid, assisted with 5 min sonication in an ultrasonic bath. These suspensions were diluted 500 times with Milli-Q water prior to spICP-MS measurements. Operating this way, the probability of two or more NPs reaching the ICP-MS detector at the same time is reduced and, hence, pulse signals are directly proportional to the analyte concentration. All the β -conglutin standards and samples were analyzed in triplicate.

2.6. ICP-MS instrumentation

All ICP-MS measurements were performed by means of an 8900 triple-quadrupole-ICP-MS system (Agilent, Santa Clara, USA) operating either in conventional or spICP-MS modes. Table 1 summarizes the ICP-MS experimental conditions for both approaches. For spICP-MS measurements, dwell time was kept at 100 μ s to reduce background and avoid the occurrence of double events [20]. The determination of β -conglutin via conventional ICP-MS detection was performed by means of a calibration curve by using the ¹⁹⁷Au⁺ ICP-MS signal response against the concentration of β -conglutin. To improve accuracy and precision, the Ir signal (¹⁹³Ir⁺) was employed as internal standard [27, 28]. For the spICP-MS detection mode, the β -conglutin calibration curve was constructed from the number of detected signal pulses (i.e., number of events) derived by NPs atomization/ionization, as previously reported by different authors [21,23]. For both calibration strategies, standards were prepared with concentrations ranging from 0.0001 to 10 nM.

Table 1
ICP-MS operating conditions for conventional and single particle modes.

	Conventional Mode	Single particle mode
Plasma forward power (W)	1550	
Argon flow rate (L min ⁻¹)		
Plasma	15	
Auxiliary	0.90	0.90
Nebulizer	1.05	0.90
Sample introduction system		
Nebulizer	MicroMist® nebulizer	
Spray chamber	Scott double pass	
Sample uptake rate (μ L min ⁻¹)	340	
Dwell time (ms)	100	0.1
Measuring time (s)	10	60
Nuclides	¹⁹⁷ Au, ¹⁹³ Ir	¹⁹⁷ Au

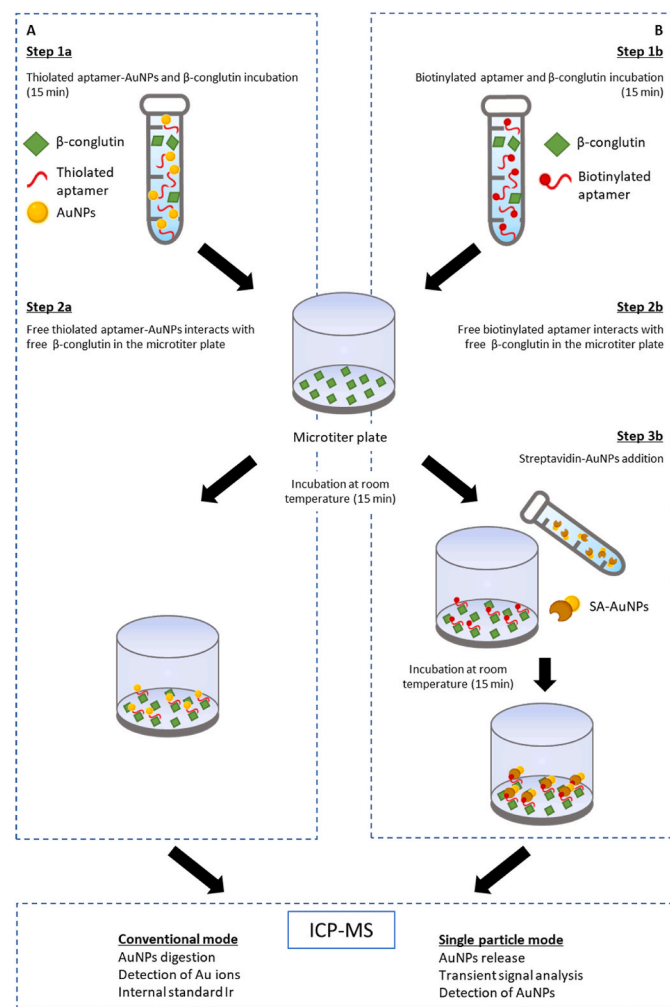


Fig. 1. Schematic of the competitive aptamer assays based on ICP-MS detection for β -conglutin determination.

2.7. Analysis of flour samples

Different pure and mixed legume flour samples (i.e., lupin, chickpea and soy) were analyzed following the procedure described by Svobodová et al. [14], with slight modifications. Briefly, 125 mg of dried sample was first defatted with 8 mL of n-hexane and then centrifuged at 6000g for 10 min at room temperature, and the pellet was dried under vacuum. The albumin fraction was then extracted from the dried pellet using 8 mL of 10 mM CaCl₂ and 10 mM MgCl₂ (pH 8.0) and then centrifuged twice at 6000g for 30 min at room temperature. To extract the conglutin fraction from the pellet, 8 mL of a solution of 100 mM Tris (hydroxymethyl)aminomethane hydrochloride (Tris-HCl) buffer (pH 7.5), 10% w w⁻¹ NaCl and 20 mM ethylenediaminetetraacetic acid was used, and then centrifuged at 6000g for 10 min at room temperature. The remaining pellet was removed, and the supernatant was diluted 100 times in binding buffer prior to analysis and used for the determination of the β -conglutin content using the developed competitive aptamer assay.

3. Results and discussion

To date, aptamer assays based on ICP-MS detection have not been widely reported. In this work, for the first time, the influence of the exogenous tag/aptamer conjugation scheme (i.e., AuNPs/thiolated aptamer and streptavidin-AuNPs/biotinylated aptamer) and ICP-MS detection mode (i.e., conventional and spICP-MS) on assay performance have been systematically investigated. Reagent concentrations (coating protein, reporter aptamer, etc.) were optimized using a type of checkerboard titration as previously described [14,27,28].

3.1. Aptamer assay based on AuNPs/thiolated aptamer

The following variables were selected for aptamer assay optimization: (i) concentration of β -conglutin for plate coating (0–180 nM); (ii) AuNPs/thiolated aptamer concentration (0.08–1.25 nM); and (iii) ICP-MS detection mode (conventional/single particle).

First, the optimization of β -conglutin concentration for plate coating was performed via a direct aptamer assay. To this end, varying concentrations of the protein in carbonate buffer were added to the wells of a microtiter plate and allowed to incubate for 30 min at room temperature. The wells were then washed three times with PBS-Tween, and an excess of the thiolated aptamer solution (5 nM) with AuNPs prepared in binding buffer was added and incubated for 15 min at room temperature. Finally, AuNPs were digested or released as described in Section 2.5.2 for detection. Fig. 2 shows the signal intensity obtained for each β -conglutin concentration used for plate coating. Irrespective of the ICP-MS detection mode (i.e., conventional or spICP-MS), the signal increased with β -conglutin concentration until a plateau was reached at 90 nM. These results were expected considering that the concentration of the coating β -conglutin used is in excess to maximize aptamer capture on the microtiter plate. Consequently, the coating β -conglutin concentration was fixed at 90 nM for further experiments.

The AuNPs/thiolated aptamer concentration was then optimized for a competitive assay (Section 2.5.1). In this case, the goal was to maximize the signal-to-background ratio (SBR) between the blank and the most concentrated β -conglutin standard (i.e., 10 nM). Because of the nature of the competitive aptamer assay, the signal achieved using ICP-MS should be maximum for a blank solution since, in the absence of β -conglutin, all the free aptamer is retained on the plate. Conversely, the signal should be minimum for standards containing a high concentration of β -conglutin in solution as minimal amounts of the aptamer would be left free for binding to the β -conglutin coated on the microtiter plate. Table 2 compiles the signal values obtained for both blank (i.e., maximum aptamer retention) and 10 nM β -conglutin standards (i.e. minimum aptamer retention) as well as the SBR values. As can be observed, the signals for the blank and 10 nM β -conglutin standards

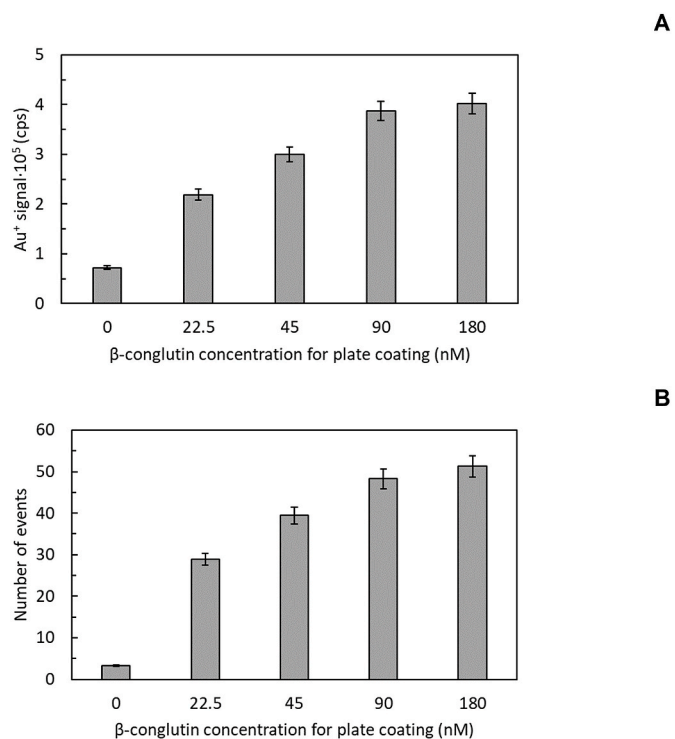


Fig. 2. Influence of coating β -conglutin concentration on analyte signal for the thiolated aptamer assay operating (A) conventional ICP-MS detection and (B) spICP-MS detection. Thiolated aptamer concentration 5 nM. Values are expressed as mean \pm standard deviation, $n = 3$.

Table 2

Influence of the thiolated aptamer concentration on analyte signal for blank and 10 nM β -conglutin standards. Conventional detection signals are expressed as Au⁺ signal in cps. Single particle ICP-MS detection signals are expressed as AuNPs number of events. Values are expressed as mean \pm standard deviation, $n = 3$.

Standard	ICP-MS (Au ⁺ signal · 10 ⁵ , cps)			spICP-MS (number of events)		
	Blank	10 nM	SBR	Blank	10 nM	SBR
Aptamer concentration (nM)						
0.08	0.34 \pm 0.04	0.10 \pm 0.02	3.4	30.4 \pm 0.7	8.5 \pm 1.4	3.6
0.15	0.52 \pm 0.06	0.12 \pm 0.04	4.3	66.6 \pm 1.0	12 \pm 2	5.6
0.30	1.66 \pm 0.04	0.20 \pm 0.08	8.3	138.7 \pm 1.2	20 \pm 2	6.9
0.60	3.88 \pm 0.14	0.64 \pm 0.12	6.1	152 \pm 2	30.8 \pm 1.4	5.0
1.25	5.1 \pm 0.4	0.92 \pm 0.06	5.5	160.0 \pm 1.5	41 \pm 3	3.9

increased with aptamer concentration, regardless of the size of the AuNPs and the ICP-MS detection mode. The signal increase observed for the 10 nM β -conglutin standard suggests the presence of non-specific interaction between AuNPs/thiolated aptamers and the microtiter plate surface [19]. Irrespective of ICP-MS detection mode, the optimum SBR was achieved using an aptamer concentration of 0.3 nM.

Using optimum operating conditions (Table 3), calibration curves for conventional and spICP-MS detection were obtained using β -conglutin standards ranging from 0.0001 to 10 nM (Fig. 3). For the sake of comparison, analytical response in Fig. 3 is expressed as the inhibition factor, defined as $(S_0 - S) \cdot 100 / S_0$ where S_0 is the maximal signal obtained with no inhibition (i.e., no β -conglutin was added) and S is the signal observed for each standard. From the corresponding calibration curves, some relevant analytical parameters were calculated for each approach,

Table 3

Optimum experimental conditions, limit of detection, half maximal effective concentration and linear range for the different aptamer assay strategies developed.

	Thiolated aptamer		Biotinylated aptamer	
	ICP-MS	spICP-MS	ICP-MS	spICP-MS
β -conglutinin plate coating concentration (nM)	90	90	90	90
Aptamer concentration (nM)	0.3	0.3	0.3	0.3
Streptavidin-AuNPs concentration ($\mu\text{g mL}^{-1}$)	-	-	5	5
LoD (pM)	200	150	2	10
EC ₅₀ (nM)	0.9	0.4	0.03	0.1
Linear range (nM)	0.2–2.0	0.1–1.2	0.001–0.08	0.015–0.9

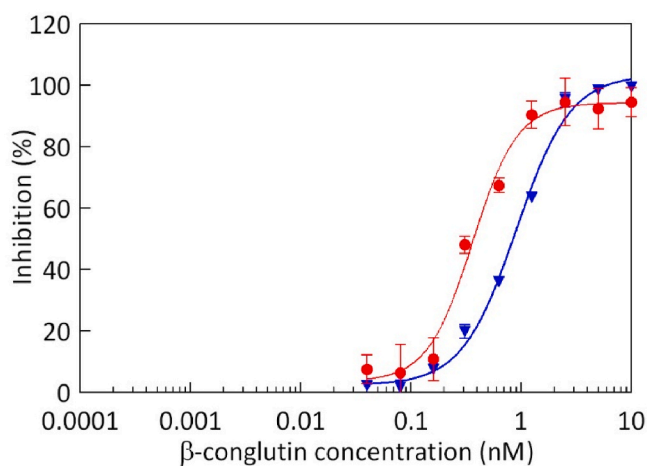


Fig. 3. β -conglutinin calibration curves for the thiolated aptamer assay using different ICP-MS detection modes: (▼) conventional detection; (●) single particle detection. β -conglutinin plate coating concentration 90 nM; thiolated aptamer concentration 0.3 nM. Error bars represent standard deviation for three replicates.

namely: (i) LoD, calculated as three times the standard deviation of the signal of 15 blank replicates [27]; (ii) half maximal effective concentration (EC₅₀); and (iii) linear range. In general, analytical figures of merit for conventional and spICP-MS detection were rather similar. The LoD obtained using the conventional mode was 200 pM. Single particle ICP-MS was observed to result in a marginal improvement in the β -conglutinin detection capability (i.e., 150 pM) as compared with the conventional mode. These results were unexpected since it has previously been observed that, for non-competitive bioassays, spICP-MS improves LoDs between 5- and 10-fold with respect to the conventional mode [21–23]. To explain these findings, it should be considered that, for non-competitive bioassays, the signal is directly proportional to the analyte concentration, and it is easier to distinguish signal pulses for low analyte standards from the blank solution. For competitive bioassays, however, it is more complex to differentiate signals between the blank and the lowest β -conglutinin standards. It must be considered that, because the high number of events detected for these solutions (Fig. S1), the uncertainty of measuring pulse frequency is significant (5–10%) thus deteriorating LoD.

3.2. Aptamer assay based on streptavidin-AuNPs/biotinylated aptamers

The optimization of this assay was carried out in the same manner as the previous procedure but modifying the SA-AuNPs concentration (1.25–10 $\mu\text{g mL}^{-1}$). The optimum β -conglutinin coating (Fig. S2) and biotinylated aptamer concentration (Table S2) for this assay were

identical to that previously observed for the AuNPs/thiolated aptamer assay and no influence of the ICP-MS detection mode was found (Table 3). Fig. 4 shows the influence of the concentration of SA-AuNPs on SBR for both conventional and spICP-MS detection modes, with 5.0 $\mu\text{g mL}^{-1}$ being optimum for both detection approaches. It is interesting to note that background signals for this approach were higher than those previously observed for the thiolated aptamer assay (Tables 2 and S2), thus suggesting higher non-specific adsorption by SA-AuNPs. Nevertheless, sensitivity is enhanced due to the higher number of AuNPs conjugated with the biotinylated aptamer thus giving rise to better SBR values. Fig. 5 shows the corresponding calibration curves for both strategies using these optimized operating conditions. As can be observed, β -conglutinin LoD using conventional ICP-MS was lower (5-fold improvement) than that achieved using spICP-MS. Moreover, it was noticed that the dynamic linear range for the latter approach was smaller (Table 3). From these results and considering previous findings for the thiolated aptamer assay, there is no clear advantage of using spICP-MS over the conventional detection mode for the competitive aptamer assays studied in this work.

Irrespective of the ICP-MS detection mode, the biotinylated aptamer assay performance was better than the thiolated one (Table 3), which can be attributed to the higher number of NPs per aptamer. The LoD obtained with the biotinylated aptamer and conventional detection were 100-fold better as compared to those obtained with the thiolated aptamer, but this improvement is limited when operating in spICP-MS mode (i.e., 15-fold). Taking these results into account, the biotinylated aptamer assay with conventional ICP-MS detection was selected for further studies.

3.3. Comparison of different methodologies for β -conglutinin determination

As there are no previous reports detailing the determination of β -conglutinin via a combination of aptamers and ICP-MS detection, the analytical parameters achieved, such as limit of detection, EC₅₀ and linear range, were compared with those reported for other aptamer assays reported in the literature (Table 4). Many of previous reports are based on the same aptamer employed in this work and, hence, it is easy to directly evaluate the benefits derived from using ICP-MS over other detection approaches (e.g., spectrophotometry UV-Vis (UV-Vis); lateral flow assay (LFA); fluorescence resonance energy transfer (FRET); real time polymerase chain reaction (rtPCR); and real time recombinase polymerase amplification (rtRPA)) [14–16]. As it can be observed, when operating with the same aptamer used in this work, the use of ICP-MS results in a 10 to 100-fold improvement in the LoD obtained. These

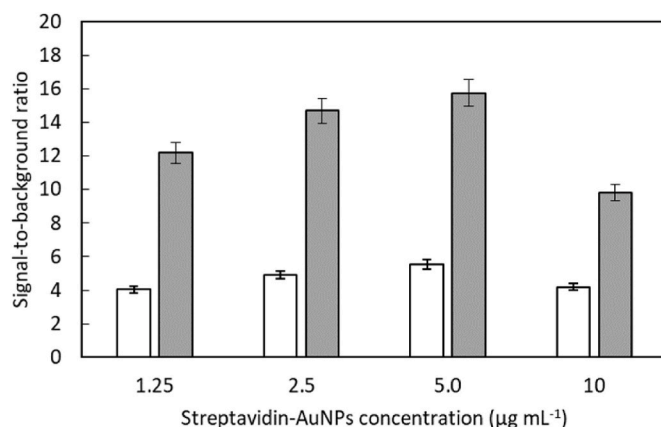


Fig. 4. Influence of SA-AuNPs concentration on signal-to-background ratio operating the biotinylated aptamer assay with conventional ICP-MS (white bars) and spICP-MS detection (grey bars). β -conglutinin plate coating concentration 90 nM; biotinylated aptamer concentration 0.3 nM. Values are expressed as mean \pm standard deviation, $n = 3$.

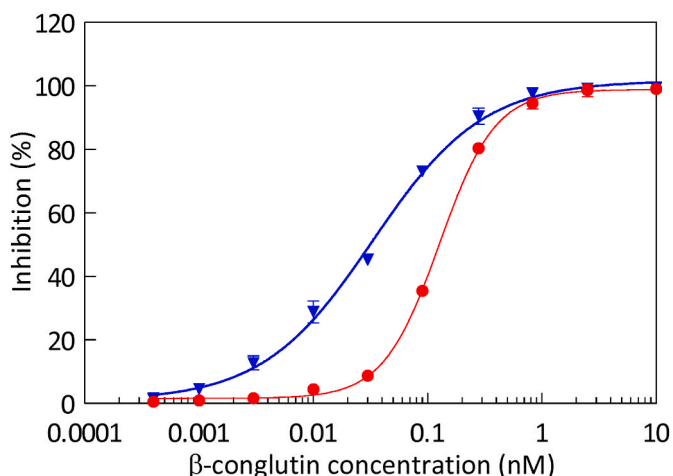


Fig. 5. β -conglutinin calibration curves for the biotinylated aptamer assay using different ICP-MS detection modes: (\blacktriangledown) conventional detection; (\bullet) single particle detection. β -conglutinin plate coating concentration 90 nM; biotinylated aptamer concentration 0.3 nM; streptavidin-AuNPs concentration $5 \mu\text{g mL}^{-1}$. Error bars represent standard deviation for three replicates.

results highlight the potential of using ICP-MS as a detector for aptamer assays. The LoD obtained were significantly higher than those achieved by the aptamer assays presented by Jauset-Rubio et al. [15] and Wu et al. [17], but these methodologies included an additional aptamer amplification/preconcentration step. It is expected that by implementing such amplification approaches as well as by increasing AuNPs size [28] or using a more sensitive spectrometer (sector field instruments) [19,35], the LoD could be further improved.

Several works have proposed the use of HPLC-MS methods for lupin determination in foods [4] but few of them have specifically focused on β -conglutinin determination. Mattarozzi et al. [36] reported a β -conglutinin detection method based on HPLC-ESI-MS/MS which afforded a LoD of 156 pM and a linear range between 0.5 and 170 nM. According to these data, our method affords better LoD (68-fold improvement) but a lower dynamic range (4-fold decrease). Nevertheless, the main benefit of using the aptamer assay with ICP-MS detection lies in sample throughput (10 s sample^{-1}), since HPLC-MS is more time consuming ($>20 \text{ min sample}^{-1}$).

3.4. Method validation for β -conglutinin in flour

The biotinylated aptamer assay based on conventional ICP-MS

Table 4
Comparison of different β -conglutinin detection strategies based on the use of aptamers.

Aptamer	Exogenous tag	Detection technique	LoD (pM)	Linear range (nM)	Reference
Biotinylated ^a	40 nm AuNPs	ICP-MS	2	0.001–0.08	This work
Thiolated ^a	13 nm AuNPs	LFA	55	-	15
Biotinylated ^a	Enzyme (HRP ^f)	LFA-RPA	0.009	-	
		UV-Vis	34000	-	16
Unmodified ^a	-	rtPCR	20	-	
		rtRPA	18	-	
		rtRPA with magnetic beads	35	-	
Biotinylated (primary) ^a	Enzyme (HRP ^f) on AuNPs	UV-Vis	0.008	-	17
Thiolated (complementary) ^b					
Biotinylated ^c	Enzyme (HRP ^f)	UV-Vis	153000	-	11
Unmodified ^c	-	PCR	85	1.3–68.4	14
Fluorophore-modified ^{d,e}	Fluorophores Alexa 488 & 555	FRET	150	5–20	12

^a 5'-agc tcc aga aga taa att aca ggg gcc ggg gtg gct cag gca agg ggt tga cct gtc gta ggg att gtt tta aca act agg ata cta tga ccc c-3'.

^b 5' - ggt ggg ggt gg-3'.

^c 5'-agc tga cac agc agg ttg gtg ggg gtg gct tcc agt tgg gtt gac aat acg tag gga cac gaa gtc caa cca cga gtc gag caa tct cga aat-3'.

^d .5'-ggt ggg ggt gg-3'.

^e .5'-ggt ggg ggt gg-3'.

^f Horseradish peroxidase enzyme.

detection has been validated for β -conglutinin determination in different flour samples according to the European Conformity guidelines for the analysis of food contaminants [37]. As there is no β -conglutinin certified material, accuracy and precision was evaluated by means of a recovery assay. To this end, chickpea and soy flour samples were spiked with known amounts of lupin flour to achieve final β -conglutinin concentration levels of 100 and 600 mg kg^{-1} (i.e., approximately 0.05 and 0.3 nM in solution). A total of six replicates were analyzed in each case and recoveries ranged in all cases from 85% to 115%. These values were within the limits established by the EU for analyte concentrations below 1 mg kg^{-1} ($-50\%/20\%$) and demonstrate method trueness. In agreement with previous works [14], the methodology developed was highly specific since no signal change was measured for unspiked chickpea and soy flour samples.

Aptamer assay repeatability (intra-day precision) was evaluated by analyzing six replicates of each sample in the same day. The relative standard deviation (RSD %) of the β -conglutinin concentration was within 4–7%. As regards aptamer assay reproducibility (inter-day precision), it was determined by analyzing six replicate samples, which were spiked with the same amount of β -conglutinin, on five consecutive days. Reproducibility values range from 5 to 10%. These values agree with previous works combining immuno- or aptamer assays with ICP-MS [27–31].

4. Conclusions

This work demonstrates the ultrasensitive detection of β -conglutinin in flour samples using a competitive aptamer assay based on ICP-MS detection. The analytical parameters achieved were dependent on the aptamer assay scheme and ICP-MS detection mode. A better LoD was achieved using biotinylated aptamers linked with streptavidin-AuNPs. According to the results obtained, conventional ICP-MS detection is more advantageous than spICP-MS detection in terms of limit of detection and linear range. Unlike previous findings for non-competitive bioassays, when operating a competitive aptamer assay based on spICP-MS, signals pulses obtained from AuNPs for less concentrated β -conglutinin and blank solutions are not easily discernible thus compromising achievable detection limits. The proposed method improves β -conglutinin LoD up to two orders of magnitude as compared to other procedures previously described in the literature. A priori, the β -conglutinin LoD could be further enhanced by using more sensitive element tags and mass spectrometer. Similarly, due to the ICP-MS multielement capabilities, it could be feasible to increase the number of food allergens simultaneously measured and, hence, sample throughput. Operating in this way, the use of ICP-MS has clear potential

as compared to current detection approaches.

CRedit authorship contribution statement

Daniel Torregrosa: Data acquisition, Formal analysis, Writing – original draft, Writing – review & editing. **Miriam Jauset-Rubio:** Methodology, Data acquisition, Formal analysis, Writing – review & editing. **Raquel Serrano:** Methodology, Data acquisition. **Marketa Svobodová:** Methodology, Data acquisition. **Guillermo Grindlay:** Conceptualization, Methodology, Formal analysis, Writing – review & editing, Supervision, Project administration. **Ciara K. O’Sullivan:** Conceptualization, Methodology, Formal analysis, Writing – review & editing, Supervision. **Juan Mora:** Formal analysis, Writing – review & editing.

Declaration of competing interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

Data availability

Data will be made available on request.

Acknowledgements

The authors would like to thank the Generalitat Valenciana (Project GV/2014/138) and the Vice-Presidency for Research and Knowledge Transfer of the University of Alicante for the financial support of this work (Projects GRE12-19 and VIGROB-050). D. Torregrosa thanks the Spanish Ministerio de Ciencia, Innovación y Universidades for the given fellowship FPU17/02853.

Appendix A. Supplementary data

Supplementary data to this article can be found online at <https://doi.org/10.1016/j.aca.2023.341042>.

References

- [1] D. Ballester, I. Zacarías, E. García, E. Yáñez, Baking studies and nutritional value of bread supplemented with full-fat sweet lupine flour (*L. Albus cv multolupa*), *J. Food Sci.* 49 (1984) 14–16.
- [2] E.W. De Penna, P. Carreño, X. Urrutia, L. López, D.J. Ballester, Sensory evaluation and acceptability of cookies enriched with sweet lupine flour (*Lupinus albus cv multolupa*), *Food Sci. (N. Y.)* 52 (1987) 1434–1435.
- [3] M. Lovik, E. Namork, C.K. Fæste, E. Egaas, The Norwegian national reporting system and register of severe allergic reactions to food, *Norsk Epidemiol* 14 (2004) 155–160.
- [4] C. Villa, J. Costa, I. Mafra, Lupin allergens: clinical relevance, molecular characterization, cross-reactivity and detection strategies, *Compr. Rev. Food Sci. Food Saf.* 19 (2020) 3886–3915.
- [5] Allergen Nomenclature, WHO/IUIS allergen nomenclature sub-committee. <http://allergen.org/viewallergen.php?aid=421>, 2008. (Accessed 7 July 2022).
- [6] European Parliament Regulation (EU), Text with EEA Relevance L304/18 C.F.R., EU, Brussel, Belgium, 2011. No 1169/2011 of the European Parliament and of the Council of 25 October 2011 on the Provision of Food Information to Consumers, Amending Regulations (EC) No 1924/2006 and (EC) No1925/2006 of the European Parliament and of the Council, and Repealing Commission Directive 87/250/EEC, Council Directive 90/496/EEC, Commission Directive 1999/10/EC, Directive 2000/13/EC of the European Parliament and of the Council, Commission Directives 2002/67/EC and 2008/5/EC and Commission Regulation (EC) No 608/2004.
- [7] D.E. Goggin, G. Mir, W.B. Smith, M. Stuckey, P.M.C. Smith, Proteomic analysis of lupin seed proteins to identify conglutin b as an allergen, *Lup an 1*, *J. Agric. Food Chem.* 56 (2008) 6370–6377.
- [8] P. Nadal, N. Candela, I. Katakis, C.K. O’Sullivan, Extraction, isolation and characterization of globulin proteins from *Lupinus albus*, *J. Agric. Food Chem.* 59 (2011) 2752–2758.
- [9] G. Huscheck, J. Bonick, Y. Lowenstein, S. Sievers, H. Rawel, Quantification of allergenic plant traces in baked products by targeted proteomics using isotope marked peptides, *LWT—Food Sci. Technol.* 74 (2016) 286–293.
- [10] L. Holden, C.K. Fæste, E. Egaas, Quantitative sandwich ELISA for the determination of lupine (*Lupinus spp.*) in foods, *J. Agric. Food Chem.* 53 (2005) 5866–5871.
- [11] P. Nadal, A. Pinto, M. Svobodová, N. Canela, C.K. O’Sullivan, DNA aptamers against the Lup an 1 food allergen, *PLoS One* 7 (2012), 35253.
- [12] T. Mairal, P. Nadal, M. Svobodová, C.K. O’Sullivan, FRET-based dimeric aptamer probe for selective and sensitive Lup an 1 allergen detection, *Biosens. Bioelectron.* 54 (2014) 207–210.
- [13] E. Lima-Cabello, J.D. Alché, J.C. Jiménez-López, Narrow-leafed lupin main allergen β -conglutin (Lup an 1) detection and quantification assessment in natural and processed foods, *Foods* 8 (2019) 513–532.
- [14] M. Svobodová, T. Mairal, P. Nadal, M.C. Bermudo, C.K. O’Sullivan, Ultrasensitive aptamer-based detection of β -conglutin food allergen, *Food Chem.* 165 (2014) 419–423.
- [15] M. Jauset-Rubio, M. Svobodová, T. Mairal, C. McNeil, N. Keegan, M.S. El-Shahawi, A.S. Bashammakh, A.O. Alyoubi, C.K. O’Sullivan, Aptamer lateral flow assays for Ultrasensitive detection of β -conglutin combining recombinase polymerase amplification and tailed primers, *Anal. Chem.* 88 (2016) 10701–107096.
- [16] M. Jauset-Rubio, J. Sabaté del Río, T. Mairal, M. Svobodová, M.S. El-Shahawi, A. S. Bashammakh, A.O. Alyoubi, C.K. O’Sullivan, Ultrasensitive and rapid detection of β -conglutin combining aptamers and isothermal recombinase polymerase amplification, *Anal. Bioanal. Chem.* 409 (2017) 143–149.
- [17] Z. Wu, D. He, E. Xu, A. Jiao, M.F.J. Chughtai, Z. Jin, Rapid detection of β -conglutin with a novel lateral flow aptasensor assisted by immunomagnetic enrichment and enzyme signal amplification, *Food Chem.* 269 (2018) 375–379.
- [18] Z. Liu, X. Li, G. Xiao, B. Chen, M. He, B. Hu, Application of inductively coupled plasma mass spectrometry in the quantitative analysis of biomolecules with exogenous tags: a review, *TrAC, Trends Anal. Chem.* 93 (2017) 78–101.
- [19] D. Torregrosa, G. Grindlay, L. Gras, J. Mora, Immunoassays based on inductively coupled plasma mass spectrometry detection: so far so good, so what? *Microchem. J.* 166 (2021), 106200.
- [20] F. Laborda, E. Bolea, J. Jiménez-Lamana, Single particle inductively coupled plasma mass spectrometry: a powerful tool for nanoanalysis, *Anal. Chem.* 86 (2014) 2270–2278.
- [21] R. Liu, Z. Xing, Y. Lv, S. Zhang, X. Zhang, Sensitive sandwich immunoassay based on single particle mode inductively coupled plasma mass spectrometry detection, *Talanta* 83 (2010) 48–54.
- [22] Y. Cao, G. Mo, J. Feng, X. He, L. Tang, C. Yu, B. Deng, Based on ZnSe quantum dots labelling and single particle mode ICP-MS coupled with sandwich magnetic immunoassay for the detection of carcinoembryonic antigen in human serum, *Anal. Chim. Acta* 1028 (2018) 22–31.
- [23] Y. Cao, J. Feng, L. Tang, G. Mo, W. Mo, B. Deng, Detection of three tumor biomarkers in human lung cancer serum using single particle inductively coupled plasma mass spectrometry combined with magnetic immunoassay, *Spectrochim. Acta, Part B* 166 (2020), 105797.
- [24] E. Pérez, K. Bierla, G. Grindlay, J. Szpunar, J. Mora, R. Lobinski, Lanthanide polymer labels for multiplexed determination of biomarkers in human serum samples by means of size exclusion chromatography-inductively coupled plasma mass spectrometry, *Anal. Chim. Acta* 1018 (2018) 7–15.
- [25] M. Careri, L. Elviri, M. Maffini, A. Mangia, C. Mucchino, M. Terenghi, Determination of peanut allergens in cereal-chocolate-based snacks: metal-tag inductively coupled plasma mass spectrometry immunoassay versus liquid chromatography/electrospray ionization tandem mass spectrometry, *Rapid Commun. Mass Spectrom.* 22 (2008) 807–811.
- [26] P. Jarujamrus R. Chawengkirtikul, J. Shiowatana, A. Siripinyanond, Towards chloramphenicol detection by inductively coupled plasma mass spectrometry (ICP-MS) linked immunoassay using gold nanoparticles (AuNPs) as element tags, *J. Anal. Atomic Spectrom.* 27 (2012) 884–890.
- [27] E. Pérez, P. Martínez-Peinado, F. Marco, L. Gras, J.M. Sempere, J. Mora, G. Grindlay, Determination of aflatoxin M1 in milk samples by means of an inductively coupled plasma mass spectrometry-based immunoassay, *Food Chem.* 230 (2017) 721–727.
- [28] E. Pérez, F. Marco, P. Martínez-Peinado, J. Mora, G. Grindlay, Evaluation of different competitive immunoassays for aflatoxin M1 determination in milk samples by means of inductively coupled plasma mass spectrometry, *Anal. Chim. Acta* 1049 (2019) 10–19.
- [29] Q. Zhao, X. Lu, C.G. Yuan, X.F. Li, X. Chris Le, Aptamer-linked assay for thrombin using gold nanoparticle amplification mass spectrometry detection, *Anal. Chem.* 81 (2009) 7484–7489.
- [30] J.M. Liu, X.P. Yan, Ultrasensitive, selective and simultaneous detection of cytochrome c and insulin based on immunoassay and aptamer-based bioassay in combination with Au/Ag nanoparticle tagging and ICP-MS detection, *J. Anal. At. Spectrom.* 26 (2011) 1191–1197.
- [31] X. Zhang, B. Chen, M. He, H. Wang, B. Hu, Gold nanoparticles labeling with hybridization chain reaction amplification strategy for the sensitive detection of HepG2 cells by inductively coupled plasma mass spectrometry, *Biosens. Bioelectron.* 86 (2016) 736–740.
- [32] D. Jiang, C. Huang, L. Shao, X. Wang, Y. Jiao, W. Li, J. Chen, X. Xu, Magneto-controlled aptasensor for simultaneous detection of ochratoxin A and fumoisin B1 using inductively coupled plasma mass spectrometry with multiple metal nanoparticles as element labels, *Anal. Chim. Acta* 1127 (2020) 182–189.
- [33] M. Jauset-Rubio, M. Svobodová, T. Mairal, T. Schubert, S. Künne, G. Mayer, C. K. O’Sullivan, β -Conglutin dual aptamers binding distinct aptatopes, *Anal. Bioanal. Chem.* 408 (2016) 875–884.
- [34] M. Jauset-Rubio, M. Svobodová, T. Mairal, C.K. O’Sullivan, Surface plasmon resonance imaging (SPRI) for analysis of DNA aptamer: β -conglutin interactions, *Methods* 97 (2015) 20–26.

- [35] D. Ardel, A. Polatajko, O. Primm, M. Reijnen, Isotope ratio measurements with a fully simultaneous Mattauch-Herzog ICP-MS, *Anal. Bioanal. Chem.* 405 (2013) 2987–2994.
- [36] M. Mattarozzi, C. Bignardi, L. Elviri, M. Careri, Rapid shotgun proteomic liquid chromatography-electrospray ionization-tandem mass spectrometry-based method for the lupin (*Lupinus albus* L.) multi-allergen determination in foods, *J. Agric. Food Chem.* 60 (2012) 5841–5846.
- [37] EC, Commission Decision 2002/657/EC of 12 August 2002 Implementing Council Directive 96/23/EC Concerning the Performance of Analytical Methods and the Interpretation of Results, as Amended by Decision 2003/181/EC (4), *Official Journal of the European Communities*, 2002, pp. 8–36.